

AETHER DIGITAL PLATFORM

WEB APPLICATION INSTRUCTIONS

For Professional Use

Version 6.0 / 2025.06.

TABLE OF CONTENTS

Release Notes.....	6
1 GENERAL INFORMATION.....	7
2 INTENDED USE.....	8
2.1 Contraindication.....	8
3 KEY FEATURES.....	9
3.1 BLE connection.....	10
4 ACCESSING THE ADP APPLICATION.....	11
4.1 Login or Setup account.....	11
4.1.1 Sign in to your account page.....	12
4.1.1.2 Login Second Step.....	13
4.1.2 Create an account page.....	14
4.1.2.2 Two factor Authentication.....	17
4.1.3 Clinician Account Deletion.....	17

- 4.1.4 Reset Password..... **18**
- 5 LANDING PAGE ONCE ACCOUNT IS SETUP..... **19**
- 5.1 Clinician dashboard..... **22**
- 5.1.2 Account Settings..... **23**
- 5.2 Connect to Zeus..... **25**
- 5.3 Patients..... **26**
- 5.3.1 Create a new patient account..... **26**
- 5.3.2 Goals..... **32**
- 5.4 Devices..... **34**
- 5.4.1 Assign a device to a Patient..... **35**
- 5.5 Medical Professionals..... **35**
- 5.5.1 List of Medical Professionals..... **35**
- 5.5.2 Invite new Medical Professional..... **36**
- 6 ZEUS CONFIGURATOR..... **38**
- 6.1 Access to Zeus Configurator..... **41**
- 6.1.1 Changing Zeus Hand Settings..... **44**

6.2 EMG Settings.....	53
6.3 Grips configuration tab.....	58
6.4 Choose grips tab.....	59
6.4.1 Custom Grips.....	60
6.5 Prosthesis settings tab.....	62
6.5.1 Input Options.....	62
6.5.2 Input Sites.....	63
6.5.3 Speed Control Strategy.....	64
6.5.4 Grip switching settings.....	68
6.5.5 Soft-Grip.....	69
6.5.6 Finger speed calibration.....	70
6.5.7 Ignore EMG spikes.....	70
6.5.8 EMG freeze mode.....	70
6.5.9 Audio & vibration signal guide.....	71
7 DEVICE USAGE MONITORING - DUM.....	73
8 MODES.....	75
9 ALLIED HEALTH.....	77

- 9.1 Allied Health permissions..... **77**
- 9.2 Allied Health – My patients..... **78**
- 10 TECHNICAL SUPPORT..... **79**
- 10.1 Troubleshooting..... **79**
- 10.1.1 Configuration not found:..... **79**
- 10.1.2 Upgrade needed:..... **80**
- 10.1.3 Firmware Update..... **82**
- 10.1.4 WIFI..... **82**
- 10.2 Compatibility..... **82**
- 10.3 Reporting..... **83**
- 10.4 Security..... **83**
- 11 OTHER INFORMATION..... **83**
- 11.1 Symbols..... **84**

Release Notes

⚠ Warning!

Date of the last update of this Software instruction: 2025.06.12

- We highly recommend reading this document carefully before using the software.
- This document contains information about the proper and safe use of the software.
- This document is regarding Aether Digital Platform v. 1.10.0 web software application [W-ADP].
- We highly recommend keeping this document in a safe place.
- If you have any questions about the product, please use the contact form on our website: www.aetherbiomedical.com

⚠ Warning!

Clinicians certified by Aether Biomedical can connect with the Zeus prosthetic hand by opening the Zeus Configurator function within the Aether Digital Platform. Do not use any third party software to connect with the Zeus hand.

⚠ Warning!

Only certified clinicians can use the Aether Digital Platform to make changes in the Zeus hand settings.

1 GENERAL INFORMATION

- Aether Digital Platform software is compatible only with the Zeus hand. All required functions are available in the Aether Digital Platform application. There is no requirement to download anything from a website to launch the program.
- The Aether Digital Platform must be accessed via Google Chrome web browser (version 131 or higher) or Microsoft Edge web browser (version 131 or higher).
- Bluetooth Low Energy 4.0 or higher version is necessary to connect to the Zeus hand.
- The Aether Digital Platform allows clinicians to set up accounts, invite other medical professionals, patients, adjust various settings and parameters of the Zeus hand remotely, allowing clinicians to customize the device for their patients.

The Aether Digital Platform allows clinicians to remotely connect with the patient through the patient mobile application (The Aether Digital Platform Mobile [M-ADP]).

The patient mobile app can be downloaded from the Apple Appstore or Google Play store.

Another functionality of the Aether Digital Platform is to render usage data of the Zeus hand and enable clinicians to adjust settings according to patient needs.

2 INTENDED USE

The Aether Digital Platform is intended to monitor the Zeus device (prosthetic hand class I device) and remotely connect with the patient.

- The Aether Digital Platform is designed to be used solely by clinicians certified by Aether Biomedical. Patients, as the users of the prosthesis, do not have access to this web based software. However, patients will have access to a mobile application.
- The software provided by Aether Biomedical is designed exclusively for the Zeus hand.
- The Aether Digital Platform enables clinicians to remotely connect with patients through the Aether Digital Platform Mobile (M-ADP) application. The app is available for download on the App Store and Google Play Store.

2.1 Contraindication

The Aether Digital Platform is not recommended for Clinicians who have not been trained by Aether Biomedical.

3 KEY FEATURES

The Aether Digital Platform (ADP) contains a web application for Clinicians and a Mobile App for Patients. The mobile App is available in both iOS and Android.

The ADP web application:

- Clinician to log into their account (if already created).
- Set up their account and login credentials for the first time. This is secure and includes two factor authentication.
- Set up a patient profile and invite the patient to the mobile app.
- Assign a Zeus hand to the patient, configure and adjust the settings of the hand to suit the personal situation of the patient.
- Allow the Clinician to set up a local, remote or asynchronous session with the patient and adjust parameters of the Zeus hand via these sessions. These sessions allow the clinician to make parameter changes to the Zeus hand and send these changes to the hand via a range of sessions either locally, asynchronously or remotely.
- **Note:** previous settings can be restored simply by loading previously saved configurations from the history logs

- Invite a fellow medical professional via the platform feature “Invite a new Medical Professional”
- The clinician can view the user’s EMG muscle contractions in real-time graphs and adjust the activation levels/ thresholds.
- Integrated within the application is the Zeus Configurator feature that allows the Clinician to input options, sites, define the hand control strategy, grip changes, grip switching modes etc.

3.1 BLE connection

The Zeus hand uses BLE (Bluetooth Low Energy) to communicate with the Zeus Configurator.

- To start configuring the Zeus, it is necessary to have the Bluetooth on your computer enabled/ switched on.

Note:

If your device does not come with an inbuilt Bluetooth modem, you can use a BLE dongle. You will need to install its drivers according to the provider’s instructions.

If you are using a Chromebook device running ChromeOS then the app may not work properly. Problems may occur when trying to connect the application using BLE.

4 ACCESSING THE ADP APPLICATION


For the best experience, we recommend using Google Chrome or Microsoft Edge. The application is compatible with systems running Windows (version 11 or higher) or Mac OS (version 14 or higher). An internet connection is required.

If you are a clinician certified by Aether Biomedical open the Aether Digital Platform at the following URL in the chosen web browser: <https://zeushand.com>

4.1 Login or Setup account


From the landing page, the Clinician has the following options:

1. Sign in if the user already has an account setup
2. Create an account
3. Reset their password if forgotten

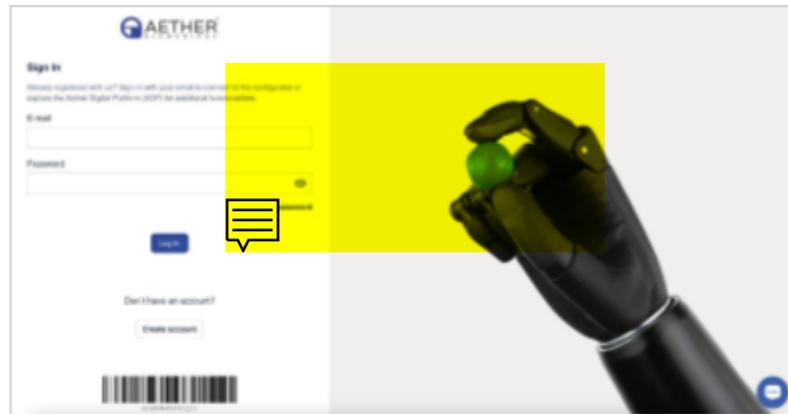

4.1.1 Sign in to your account page

If you already have an account setup, follow the screen below to log into your account.

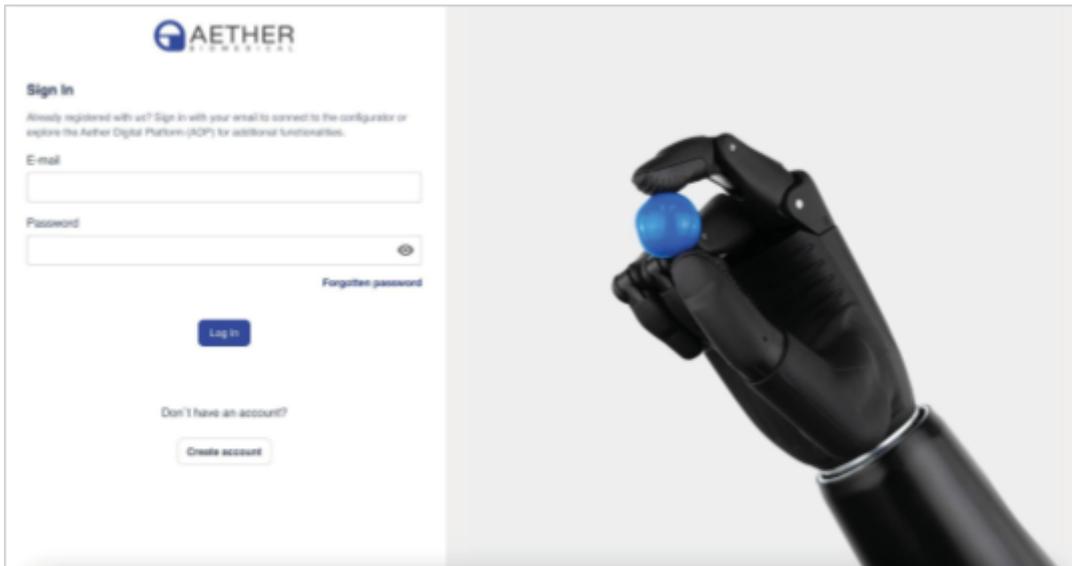

AETHER
BIOMEDICAL

Sign In

Already registered with us? Sign in with your email to connect to the configurator or explore the Aether Digital Platform (ADP) for additional functionalities.

E-mail

Password

[Forgot password](#)


[Log In](#)

Don't have an account?

[Create account](#)

4.1.1.2 Login Second Step

For users who have enabled Two-Factor Authentication (2FA), the second step of the login process requires entering a verification code. This code is sent to your verified mobile device or email, depending on your selected authentication method.

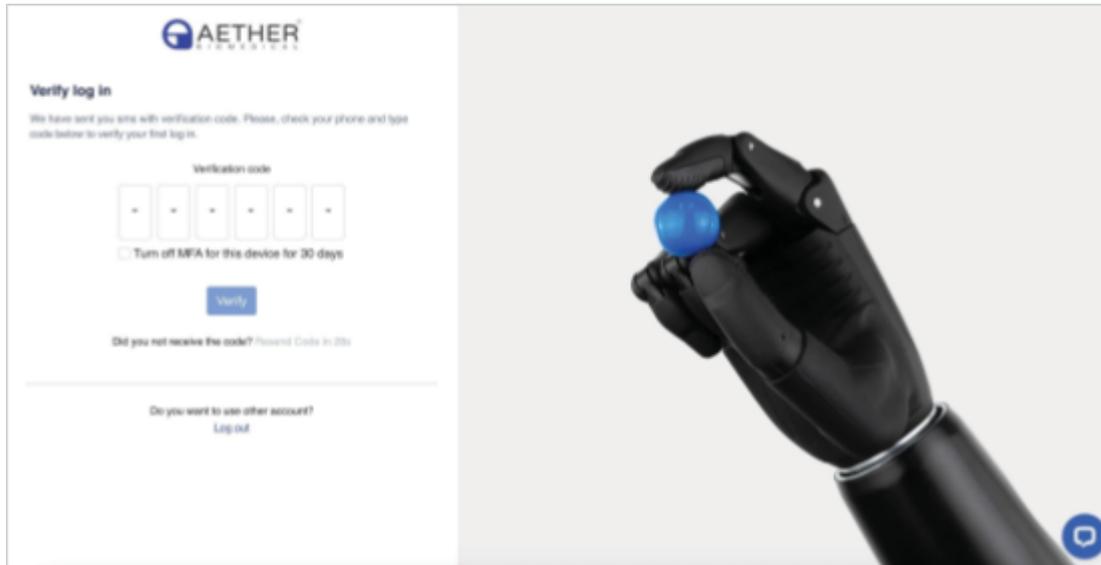

4.1.2 Create an account page

AETHER

Create account

Set up an account in three simple steps. Fill information below and add activation code to continue registration.

Basic Info Activation Code Client's Info

Basic Info

Name

E-mail

Phone Number

+44

Password

The password should contain at least 8 characters, and combine letters, one number, one uppercase letter, one special character.

Re-type Password

Language


Region


Choose the region where your data will live.

I agree [Terms of Service](#)

I agree [Privacy Policy](#)


If you do not yet have an account setup, click on the "Create Account" button on the landing page and follow the process in the screens below

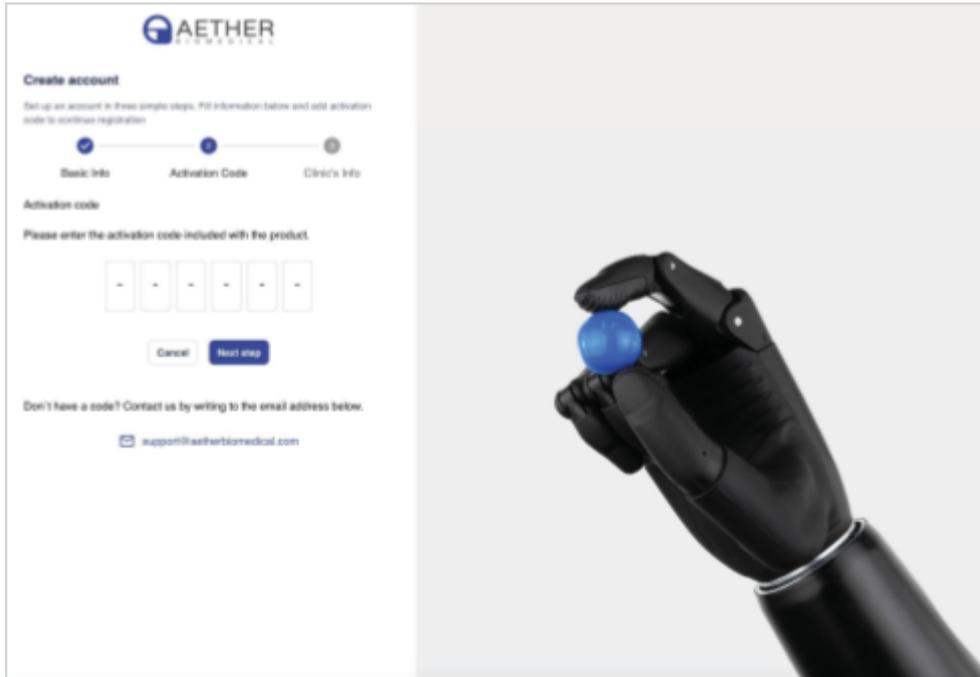

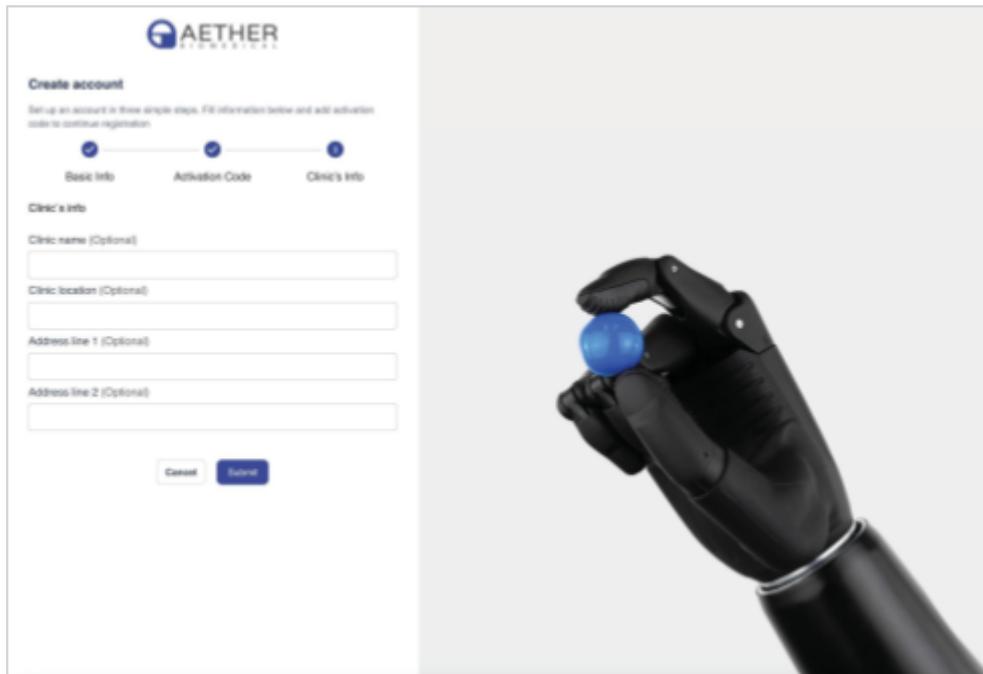

Note:

- Please ensure to select your region correctly, e.g. if a US clinician, select USA. Your data and that of patients under your care will be stored in the region selected.
- You will need to enter the Activation Code received with the Zeus hand. Please enter this as indicated in the image on the right hand side.

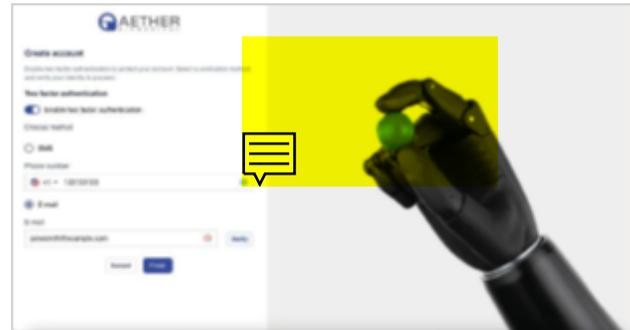

4.1.2.2 Two factor Authentication

In order to provide an additional layer of account security, we recommend you enable two factor authentication (2FA) with either email or a phone number.


Note: Two factor authentication is enabled by default in the design

4.1.3 Clinician Account Deletion

Please contact Aether Biomedical support on support@aetherbiomedical.com to delete your account.

4.1.4 Reset Password


To reset your password, click the 'Reset Password' button to be redirected to the reset password page. Enter your email address, submit the request, and wait for an email containing the password reset link.

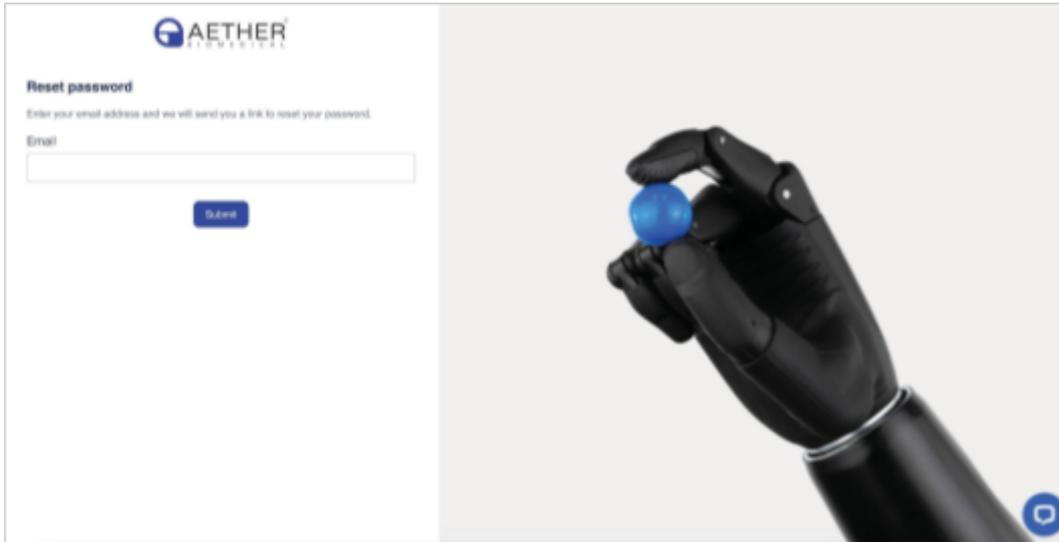


The image shows a screenshot of the Aether Biomedical website's password reset interface. On the left, the Aether Biomedical logo is at the top. Below it, the heading "Reset password" is followed by the instruction "Enter your email address and we will send you a link to reset your password." There is a text input field labeled "Email" and a blue "Submit" button. On the right, a black robotic hand is shown holding a blue sphere, with a small blue circular icon in the bottom right corner of the image area.

5 LANDING PAGE ONCE ACCOUNT IS SETUP

Once the account is successfully created the Clinician will receive an email with the message below.

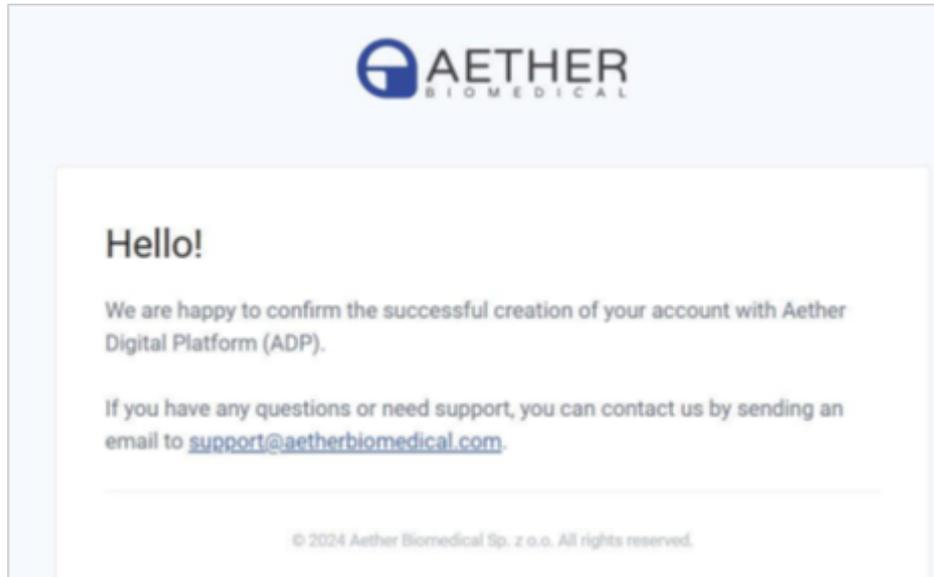


Once they login to the ADP application, the Clinician will see the screen below

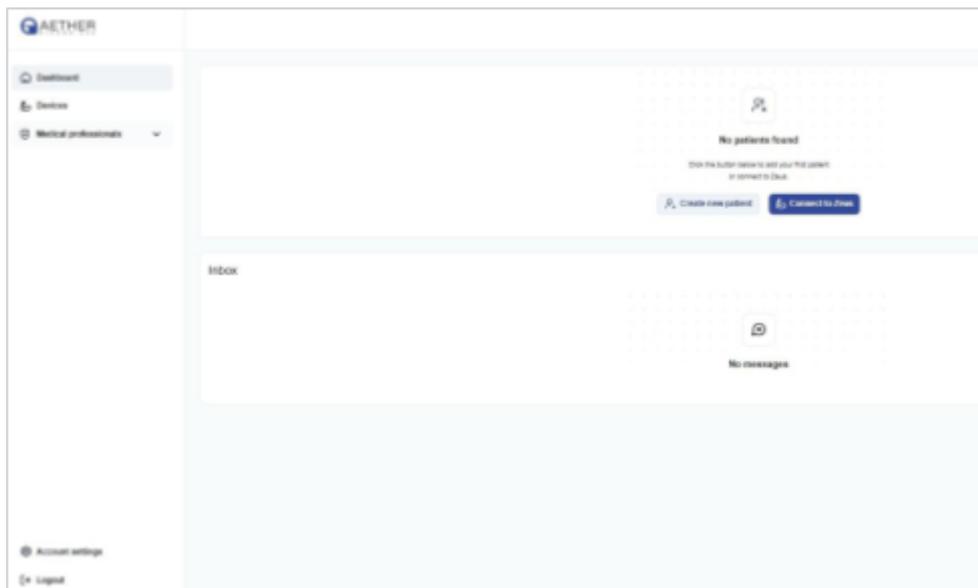

From the left hand side of this main page allows the Clinician to

- See a patient dashboard
- See Zeus Devices
- See list of medical professionals
- See Aether Academy
- Edit Account settings
- Logout from the application

From the main body of the page the Clinician can create a new patient account or connect to a Zeus Hand to begin the configuration of it.

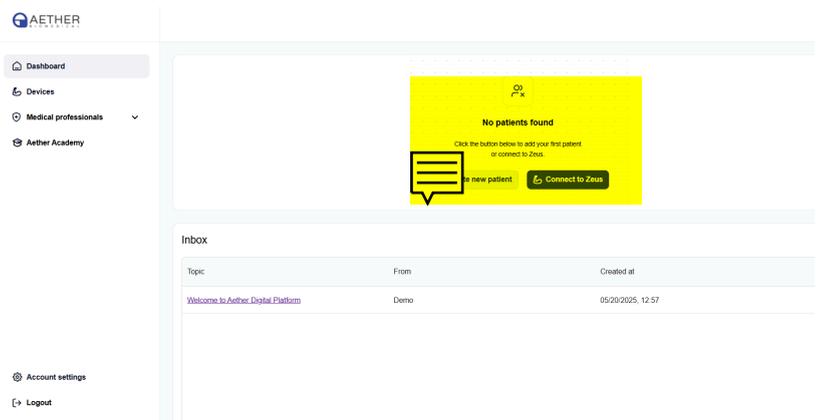


The screenshot displays the Aether Digital Platform web interface. On the left is a navigation sidebar with the following items: Dashboard (selected), Devices, Medical professionals (with a dropdown arrow), Aether Academy, Account settings, and Logout. The main content area is divided into two sections. The top section features a yellow background with the text 'No patients found' and a call to action: 'Click the button below to add your first patient or connect to Zeus.' Below this text is a 'Connect to Zeus' button. The bottom section is titled 'Inbox' and contains a table with the following data:

Topic	From	Created at
Welcome to Aether Digital Platform	Demo	05/20/2025, 12:57

5.1 Clinician dashboard

In the Clinician Dashboard, users have access to a list of patients, an inbox for messages, and a sidebar on the left for navigating through the application.

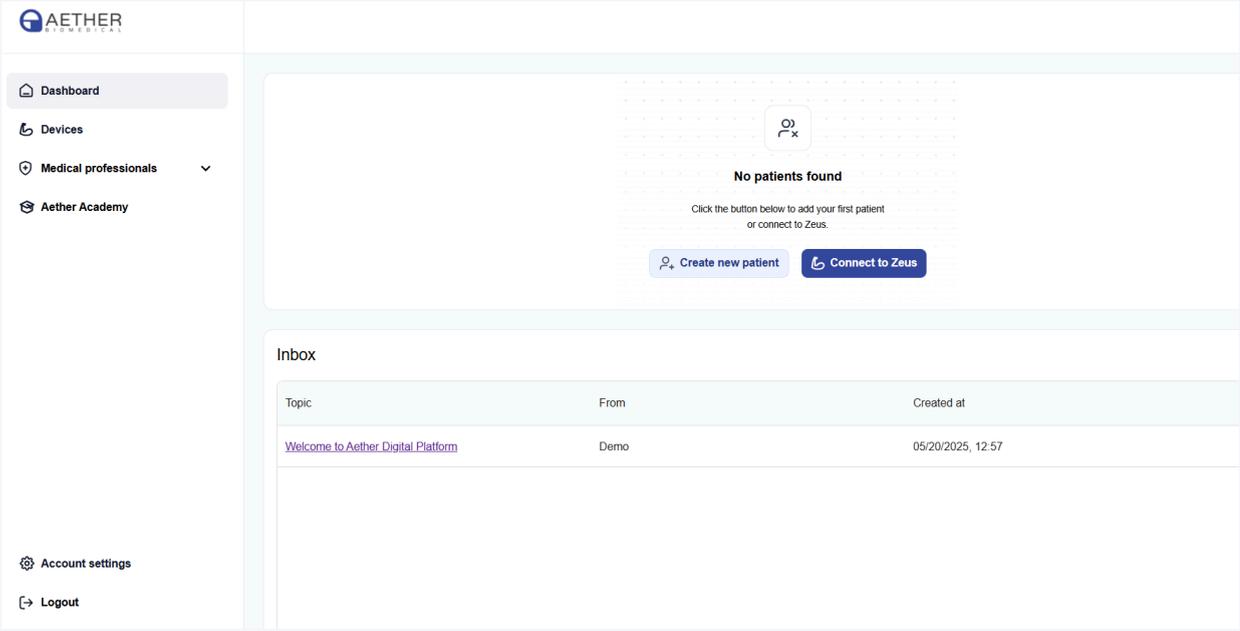

The screenshot displays the Aether Clinician Dashboard. On the left is a sidebar with the AETHER logo at the top. Below the logo are navigation items: Dashboard (selected), Devices, Medical professionals (with a dropdown arrow), and Aether Academy. At the bottom of the sidebar are Account settings and Logout. The main content area is divided into two sections. The top section, titled 'Patients', shows a 'No patients found' message with a person icon and a plus sign. Below the message is the text 'Click the button below to add your first patient or connect to Zeus.' and two buttons: 'Create new patient' and 'Connect to Zeus'. The bottom section, titled 'Inbox', contains a table with the following data:

Topic	From	Created at
Welcome to Aether Digital Platform	Demo	05/20/2025, 12:57

5.1.2 Account Settings

In User Settings, you can update your personal details and clinic information like:

- Change the account name
- Change the email address - this action will require additional confirmation by clicking on the appropriate link that will come to the new email address
- Change the telephone number - in order to verify the new number, we will send a one-time authorization code to the provided telephone number. Enter it to confirm the operation
- Change password - the action requires entering the current password; only then is it possible to set a new password.
- Enable / Disable two factor authentication - there are two methods of providing the authorization code.
- Email method - a one-time access code will be sent to the previously verified email address, which will be valid for 15 minutes from the moment of sending. After this time, the code will be invalid and a new one would have to be generated.
- Text message method (SMS) - available only when a phone number is entered

Account settings

Name
Jane Smith

Email
janesmith@example.com

Phone number
+1 123123123

Password
Change password

Language
English

Optional fields

Clinic name

Clinic location

Address Line 1

Address Line 2

Two factor authentication

Enable Two factor authentication

To deactivate your account, please contact us via email: support@aetherbiomedical.com

Save Changes


The image shows a screenshot of the 'Account settings' page. A large yellow rectangular highlight covers the right side of the page, including the 'Name', 'Email', 'Phone number', 'Password', and 'Language' sections. A callout box with three horizontal lines is positioned over the 'Language' dropdown menu, which is currently set to 'English'. The 'Optional fields' section contains four empty text input boxes for 'Clinic name', 'Clinic location', 'Address Line 1', and 'Address Line 2'. The 'Two factor authentication' section has a radio button next to the text 'Enable Two factor authentication'. At the bottom of the form is a blue button labeled 'Save Changes'. At the very bottom of the page, there is a line of text: 'To deactivate your account, please contact us via email: support@aetherbiomedical.com'.

5.2 Connect to Zeus

To connect Zeus Hand, click the blue button located in the top right corner.



This will open a Bluetooth pairing window displaying available devices. Select Zeus Hand from the list and click Connect to establish the connection.

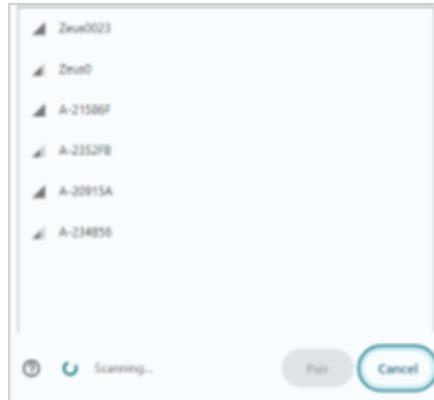

5.3 Patients

5.3.1 Create a new patient account

Create new patient

1 ————— 2

Patient Details
Please provide patient's basic information

Medical Professionals
Invite other medical professionals (CPO's OT/PT, etc. to access patient)

First Name

Last Name


E-mail


Password (Optional)

Device (Optional)

[Continue](#)


Two options exist for the clinician to create a patient account

 Creation of an account without a Zeus hand

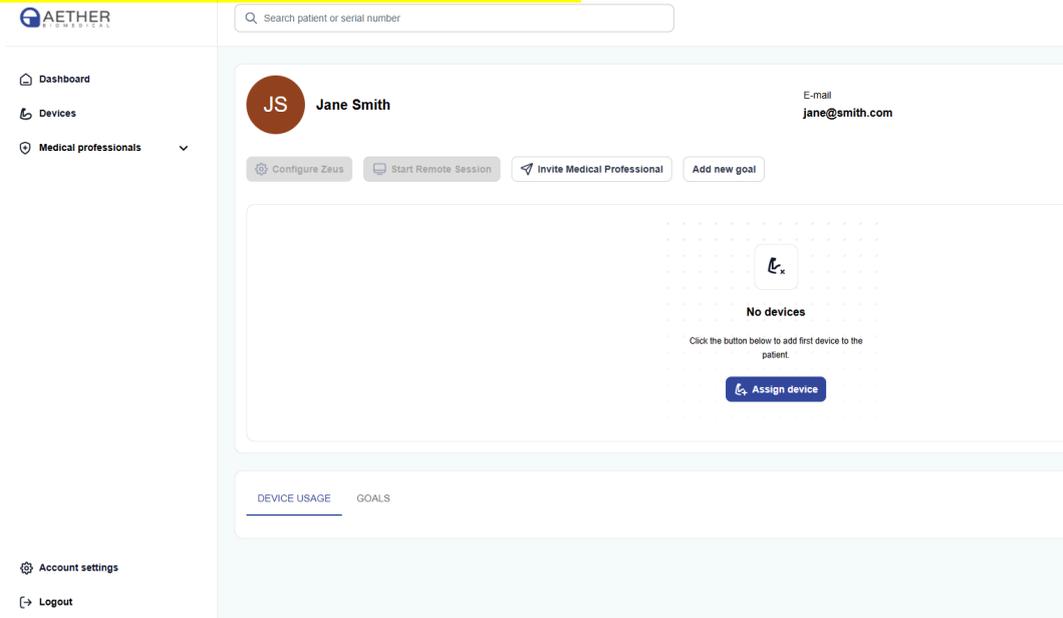

The screenshot shows the Aether Digital Platform interface for a patient profile. On the left is a navigation sidebar with the AETHER logo at the top, followed by menu items: Dashboard, Devices, Medical professionals (with a dropdown arrow), Account settings, and Logout. The main content area features a search bar at the top with the placeholder text "Search patient or serial number". Below the search bar is the patient's profile information: a circular profile picture with the initials "JS", the name "Jane Smith", and the email address "E-mail jane@smith.com". A row of action buttons is displayed: "Configure Zeus", "Start Remote Session", "Invite Medical Professional", and "Add new goal". The central part of the page shows a "No devices" message with a sub-message: "Click the button below to add first device to the patient." and a prominent blue "Assign device" button. At the bottom of the main content area, there are two tabs: "DEVICE USAGE" (which is selected) and "GOALS".


2. Creation of an account with a Zeus hand

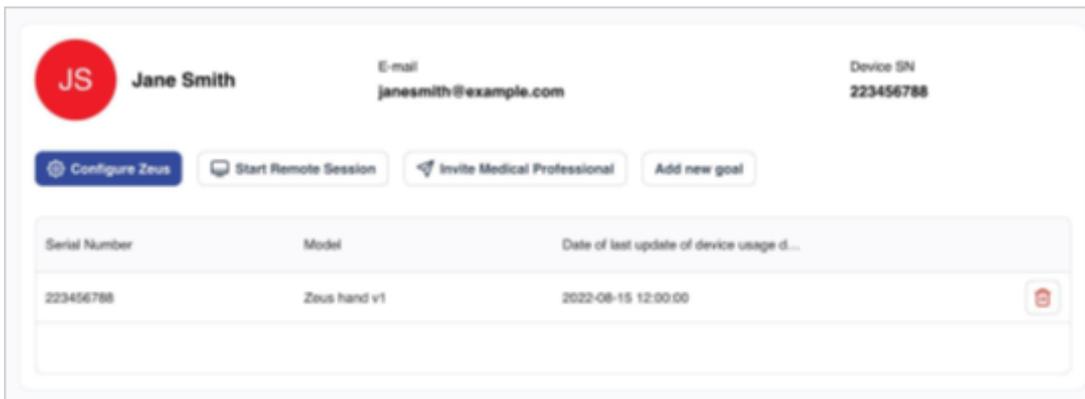

The screenshot displays a user profile for Jane Smith. At the top left is a red circular profile picture with the initials 'JS'. To the right of the profile picture, the name 'Jane Smith' is displayed. Further right, the email address 'janesmith@example.com' is shown. On the far right, the 'Device SN' is listed as '223456788'. Below the profile information, there are four buttons: 'Configure Zeus' (blue), 'Start Remote Session' (light blue), 'Invite Medical Professional' (light blue), and 'Add new goal' (light blue). Below the buttons is a table with three columns: 'Serial Number', 'Model', and 'Date of last update of device usage d...'. The table contains one row of data: '223456788', 'Zeus hand v1', and '2022-08-15 12:00:00'. A small red trash icon is visible in the bottom right corner of the table row.

Serial Number	Model	Date of last update of device usage d...
223456788	Zeus hand v1	2022-08-15 12:00:00

Once a patient is selected the window shown below will appear. From this the Clinician can then configure the Zeus hand if the Patient is in their office locally, initiate a remote session with the Patient, add new goals for the Patient or invite another medical professional into the Patient's plan.

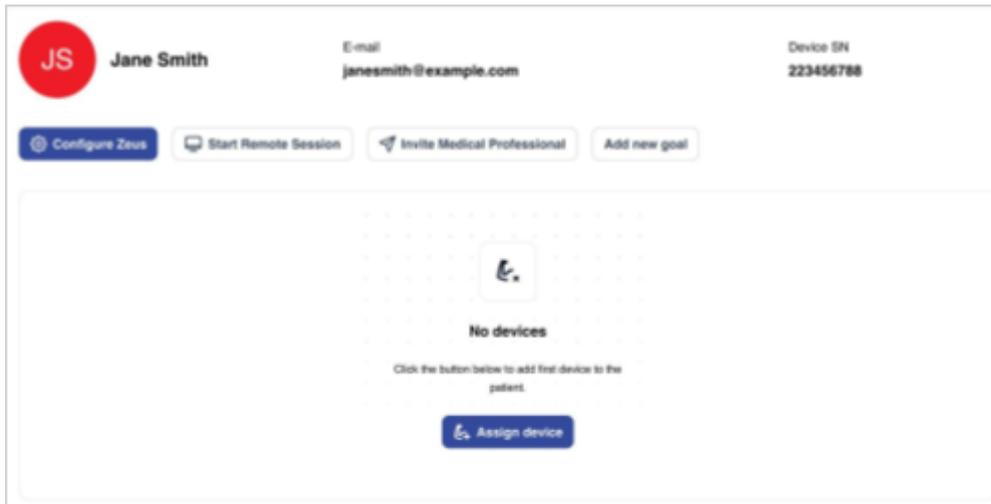

The user profile card for Jane Smith includes a red circular avatar with the initials 'JS', her name, email address 'janesmith@example.com', and device SN '223456788'. Below the profile information are four buttons: 'Configure Zeus', 'Start Remote Session', 'Invite Medical Professional', and 'Add new goal'. A table below the buttons lists device information.

Serial Number	Model	Date of last update of device usage d...
223456788	Zeus hand v1	2022-06-15 12:00:00

The 'Assign Device' dialog box features a dropdown menu labeled 'Device' with the text 'Choose from list'. Below the dropdown is a list of device IDs: '0021004', '0023002c', and '00230024'. An orange callout bubble next to the first device ID reads 'Assigned to Patrick Shad'.

The **My patients** tab shows a list of patients whose data and configurations the Clinician has access to, whether created by them or invited by another clinician.

To see patient information click on the Profile button under the Patient's name From this Patient view, the Clinician can:

- connect to the Patients Zeus Hand in a local or asynchronous session
- start a remote session
- invite another medical professional to access this patient
- add Goals for the patient
- see the list of devices and remove the device from the patient
- check the patients Device Usage Monitoring (DUM) statistics

The patient details page opens up, providing details associated with patients and hands that are linked to patients. This is also where you can access a remote session to communicate with a patient.

Clinicians and Allied health will receive e-mail when there will be a new message to read. Patients will receive push notifications on the mobile app.

5.3.2 Goals

When "Add goal " is chosen you will go directly to the form where you can set up the goals for the patient.

Add goal

1 — 2 — 3 — 4
Time frame Grips Switches Exercises

Set up time frame for goal

Choose first day

How many days will this goal take?

Goal end date calculated from the date above
28/01/25

Step 1:

In step one, choose how long this goal will last. Set the date of the first day and indicate how many days it should last.

Step 2:

In this step, you can set goals for the patient regarding grips. First, choose the frequency at which you want to start counting the number of grips performed (daily, weekly, monthly, or for the entire date range selected for the goal). You can choose the grip details whether the patient is to perform a total number of grips or a certain number of grips. You can set both of these goals at the same time. The sum of the specific grips cannot be greater than the goal for the "Total grips" count.

Step 3:

As in step 2, you indicate here the frequency and number for the grip switches. You can set a different frequency than for the grips

Step 4:

In the last step, you can choose which exercises the patient should perform. You can set the number of repetitions and frequency for each exercise separately. If you would like to add some exercises please write to us.


Under the Goals tab, you can find information about the history of goals set and completed. By clicking on the plus icon you can see the full information. Clicking on the eye icon takes you to the settings preview. The trash icon removes the goal from history.

There are 3 charts available in the goal history.

These charts outline the specific goals that the clinician selected for the patient, such as number of grips performed, frequency, and exercises.

5.4 Devices

Under the Devices tab, the Devices List displays all devices assigned to the clinician. Devices might already be assigned to a patient. This section also allows users to reassign devices to a different patient if needed

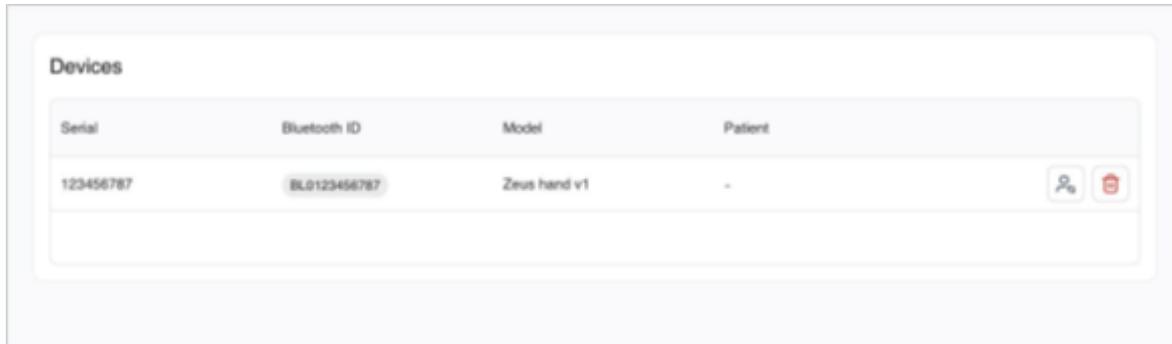

Serial	Bluetooth ID	Model	Patient	
123456787	BL0123456787	Zeus hand v1	-	 

5.4.1 Assign a device to a Patient

The device is assigned to the patient during the account creation flow.

From the same Edit device menu you can also change the Patient assigned to the device. The hand can only be assigned to one patient at a time.

5.5 Medical Professionals

5.5.1 List of Medical Professionals

Under this tab, the Clinician can view the list of medical professionals in their network. This typically be a medical professional in their network who works with a common patient to both or another medical professional the Clinician wishes to bring into the medical care delivery to the Patient.

5.5.2 Invite new Medical Professional

Invite new Medical Professional

Patient

 Jennifer Doe (jennifer@test.pl) ▼

Role ⓘ Assign Person

Clinician ▼ johnsmith@example.com ×

The Medical Professional is not in your Medical Professionals list and will be invited

[+ Add next person](#)

I confirm that the user I invited has been trained in the use of the application and is competent to do so.

A clinician can invite another clinician or medical professional even from outside their own organisation. The process of doing this is captured below.

Once invited, the invited medical professional will be able to assist and manage the patient's account.

Note: Prior to inviting the medical professional, the invitee needs to have received training on the Zeus hand and ADP.

The ADP shall allow a clinician to invite up to a maximum of ten (10) medical professionals in one time. The invitation is valid for 24 hours, after which it must be resent.

The Clinician can view the medical professionals they have added and the status of the invite.

Name	E-mail	Role	Patients	Status
Invited user	janedoe@example.com	Clinician	Jane Doe	Active
Invited user	jdndoe@example.com	Clinician	John Doe	Invitation expired
Invited user	janesmith@example.com	Clinician	Jane Smith +1	Invitation expired
Invited user	tomsmith@example.com	Allied Health	Tom Smith	Invitation expired
Invited user	saradoe@example.com	Clinician	Sara Doe	Invitation expired
Invited user	kevinsmith@example.c...	Clinician	Kevin Smith	Invitation expired

6 ZEUS CONFIGURATOR

Our concept at Aether Biomedical was to create multi-functionality in communicating and accessing the Zeus hand through multiple sessions. This will allow the greatest amount of freedom and flexibility for you and your patients.


Our multi-functional communication tool has 3 perspectives aka 3 sessions.

- Local,
- Asynchronous
- Remote Session.


1. A Local session can be accessed using the ,Connect to Zeus' button in the top-right corner of the dashboard.



- An Async session can be accessed using the ,Configure Zeus' button located in the patient card.

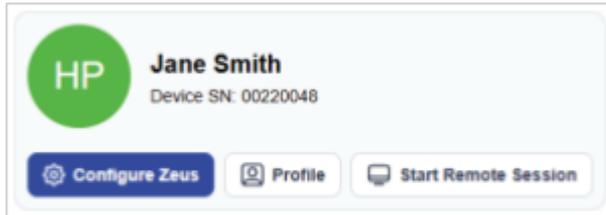

- A Remote session can be accessed using the ,Start Remote Session' button located in the patient card.

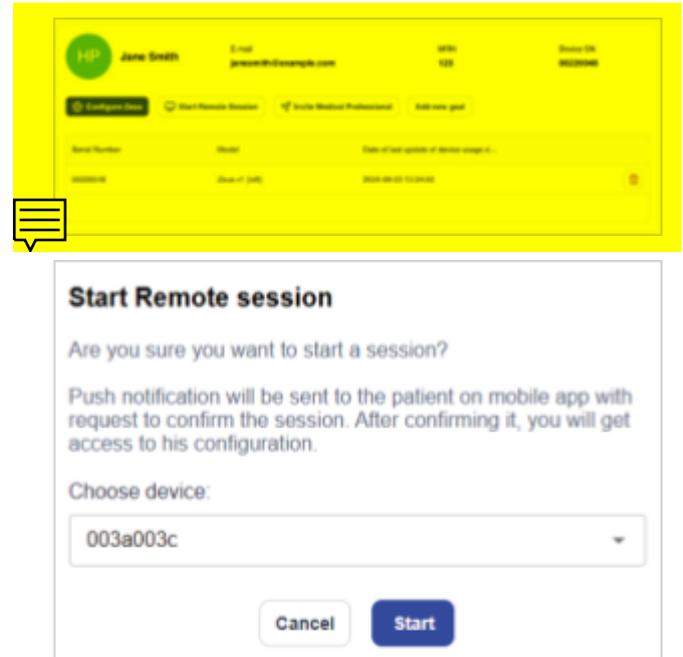


These 3 sessions give clinicians and patients flexibility and freedom to either have changes made to their Zeus hand locally (in-person at the prosthetist's clinic) or remotely.

A device registered in the ADP (Aether Digital Platform) can be configured in the following ways:

- Local Session- standard, in office configuration, where the clinician connects to the device via Bluetooth without the need of a patient to use the mobile app.
- Asynchronous Session - remote configuration, during which a clinician can propose changes to the device in the patient's absence, generating a ticket to the patient, awaiting their acceptance. For example: the patient sends the clinician a message stating that they are having difficulty with Co-contraction and wanting to change to Open-Open. The clinician will create a configuration file and send it to the patient's inbox on their mobile app. When the patient logs in to the mobile app they can then download the file to their hand.
- Remote Session - a way of simulating a face-to-face meeting with a clinician. The clinician sends an invitation to the session, to which the patient can connect via the mobile app. The built-in conferencing allows a video meeting, where the clinician can see the patient's EMG signals..
 - If the clinician closes the remote session, the changes are applied immediately. A ticket is created, and the previous settings can be restored from it.
 - If the patient closes the session, a popup appears with the question, „Do you want to save the configuration?“ They can choose to save it or load the previous settings.

6.1 Access to Zeus Configurator

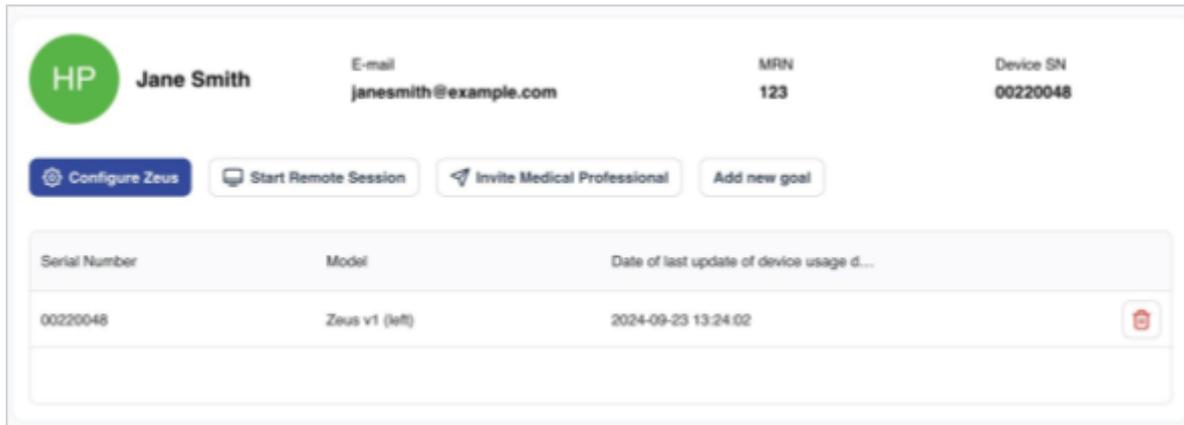

The screenshot displays a patient card for Jane Smith. At the top left is a green circular profile picture with the letters 'HP'. To its right, the name 'Jane Smith' is shown. Further right, the email address 'janesmith@example.com' is listed. On the far right, the MRN '123' and Device SN '00220048' are displayed. Below the patient information, there are four action buttons: 'Configure Zeus' (highlighted in blue), 'Start Remote Session', 'Invite Medical Professional', and 'Add new goal'. Below the buttons is a table with three columns: 'Serial Number', 'Model', and 'Date of last update of device usage d...'. The table contains one row of data: '00220048', 'Zeus v1 (left)', and '2024-09-23 13:24:02'. A small red trash icon is visible at the end of the row.


Serial Number	Model	Date of last update of device usage d...
00220048	Zeus v1 (left)	2024-09-23 13:24:02

The Zeus Configurator can be launched from the Patient card, by selecting the “Configure Zeus” Button. Allied Health is granted access to Zeus Configurator functionality in accordance with the permission granted by the Clinician.

After launching the program, the main screen of the Zeus Configurator will show up.

This main screen is divided into a number of parts:

1. Side Bar containing the following options
 - a. Grip
 - i. Choose Grips
 - ii. Configuration
 - b. EMG
 - i. Settings
 - c. Prosthesis
 - i. Prosthesis Settings
 - d. Devices
 - i. History Log
 - ii. Config Templates
 - iii. Update

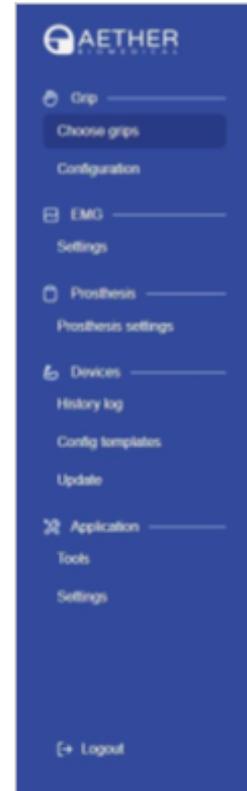

- e. Application
 - i. Tools
 - ii. About
 - f. Logout
2. Top Bar
 - a. Device Serial Number of the connected Zeus Hand
 - b. Option to "Connect to Device"
 - c. Option to "Go to ADP"
 3. Main page body showing Grips options in opposed and non-opposed modes

In the Settings Area you can change the settings of the Zeus hand. Its content depends on the currently chosen tab in the main menu.


In the Application Settings, you can check the software version, view Bluetooth Module details, and send changes to the hand settings.

Side Buttons enable you to save settings to the prosthesis, restore most recent versions of the settings, and undo the last change in the settings.

6.1.1 Changing Zeus Hand Settings

Settings for the Zeus hand can be adjusted via the Zeus Configurator. By selecting Configurator, it gives access to a menu of setting options on the left hand of the screen as shown below.

Parameters of the hand configuration which can be changed include the EMG Settings, Grips configuration, Zeus hand Prosthesis settings.

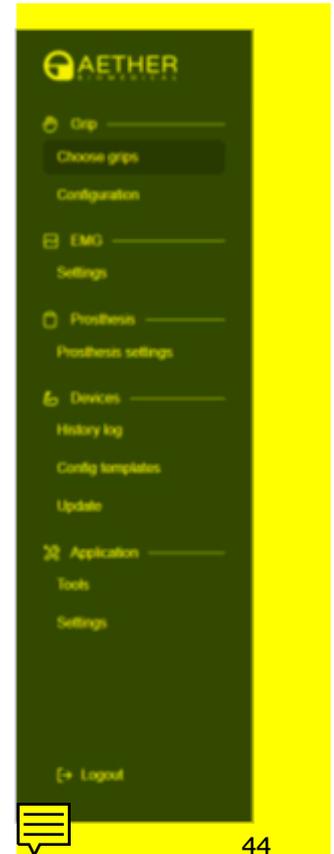

Grips Tab


In the upper right corner of the Settings Area you will find Pairing Mode/ Sequential Mode switch. Changing this switch will select the corresponding control mode setting in the prosthesis.


6.1.1.2 Choosing the control mode changes the displayed graphics in the Settings Area. There you can select the order in which the grips will be accessed in each of the control modes.

6.1.1.3 The Zeus has 14 grip patterns. The clinician can choose the grips that are the most useful in the patient's daily life.

Choose grips [ⓘ]

✓ Pairing mode Sequential mode

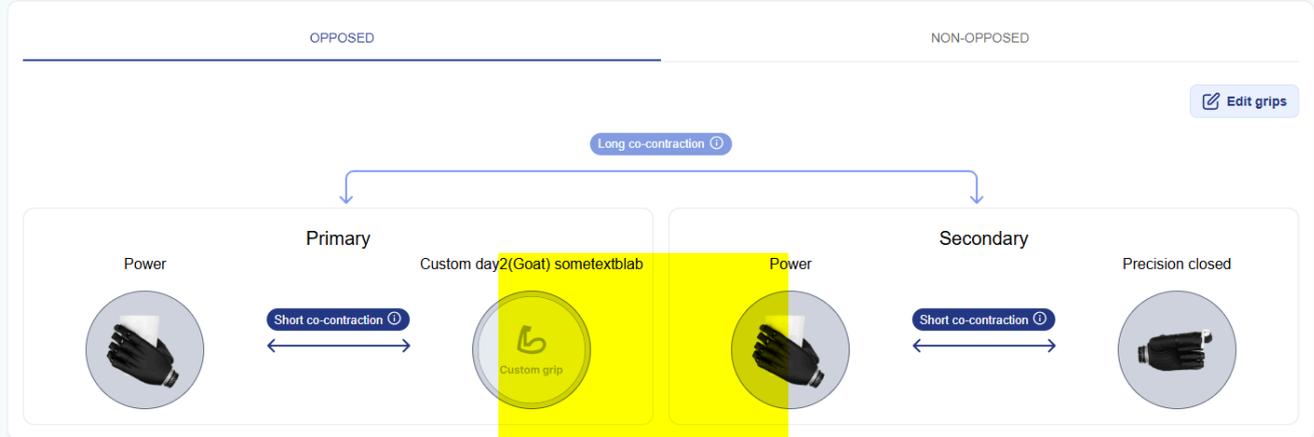


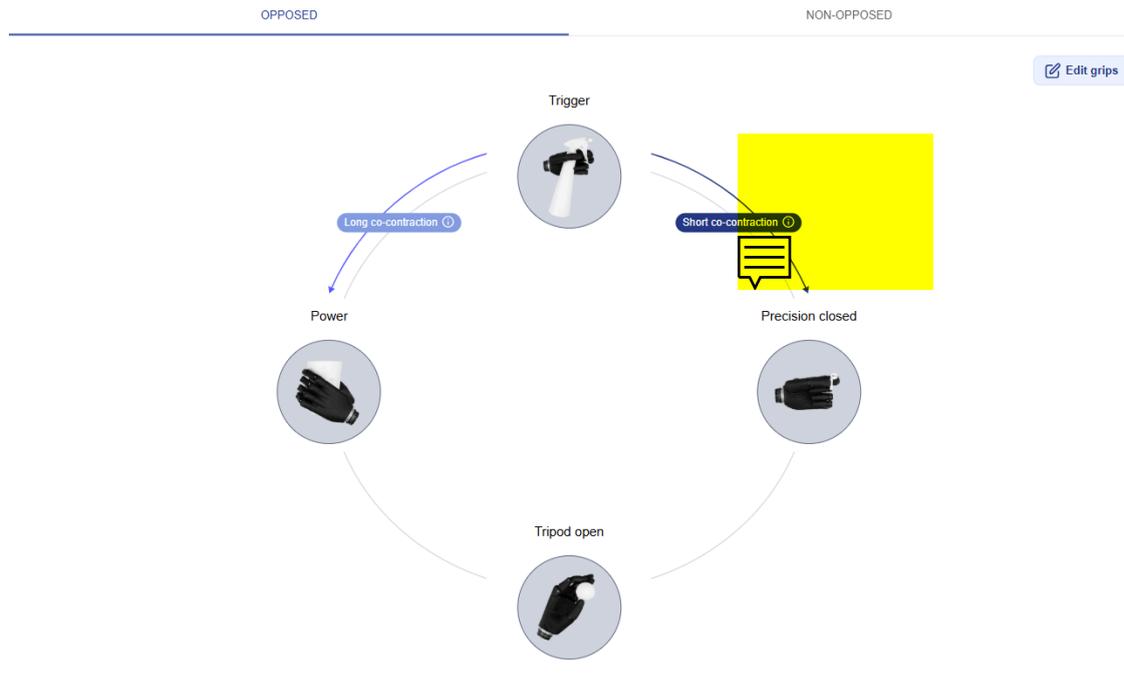

Pairing Mode

Choose grips ^①

✓ Pairing mode Sequential mode

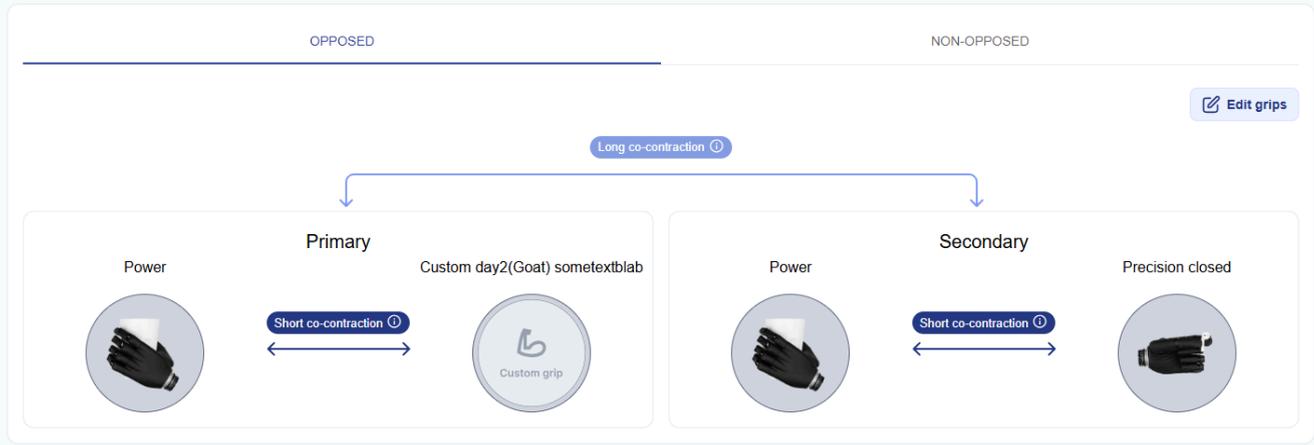

- 6.1.1.4 In Pairing Mode, the grips are arranged in a hierarchical manner, allowing for quick access. The first level of division is based on the position of the thumb. When the thumb is in the opposed position, the opposed group of grips is active and when the thumb is in the non-opposed position, the non-opposed group of grips is active.
- 6.1.1.5 To switch between the opposed group of grips and the non-opposed group of grips, the user has to move the thumb into the desired position and then provide a Change Signal.
- 6.1.1.6 Within each group of grips, there are two subgroups - the primary group and the secondary group. Each subgroup has two grips within it: the default grip and the alternate grip.
- 6.1.1.7 To switch between the default grip and the alternate grip, provide a Change Signal.
- 6.1.1.8 To switch between the subgroups, primary group and the secondary group, provide a Secondary Change Signal.
- 6.1.1.9 When you change the position of the thumb, provide a Change Signal to allow the prosthesis to change between the opposed and non-opposed group of grips.

Change Signals

The table below shows what type of signal is treated as a Primary Change Signal and Secondary Change Signal in different grip switching modes.


Grip switching mode	Primary Change Signal	Secondary Change Signal
Co-contraction	Co-contraction	Long co-contraction
Open-open	Open open	Open open open
Hold-open	Hold open	Long hold open
Single electrode alternating	Open open	Open open open
Single electrode slope	Hold open	Long hold open

Sequential Mode

In Sequential Mode you can cycle between the grips in the loop. Using the primary grip Change Signal you go forward in the loop; using the secondary grip Change Signal, you go back. The grips are split into two groups: with the thumb opposed and non-opposed. To switch between the groups, you need to manually adjust the thumb position and generate a grip Change Signal or a secondary grip Change Signal.

The order and number of grips of each of the groups can be modified after selecting "Sequential Mode" in the Settings Area.

In Sequential Mode there can be a maximum of 5 grips in each of the groups defined by the thumb position. This number can be decreased by unchecking the last grip in the group - the unused grip will be greyed out. You can re-activate the grip by checking the box over it.

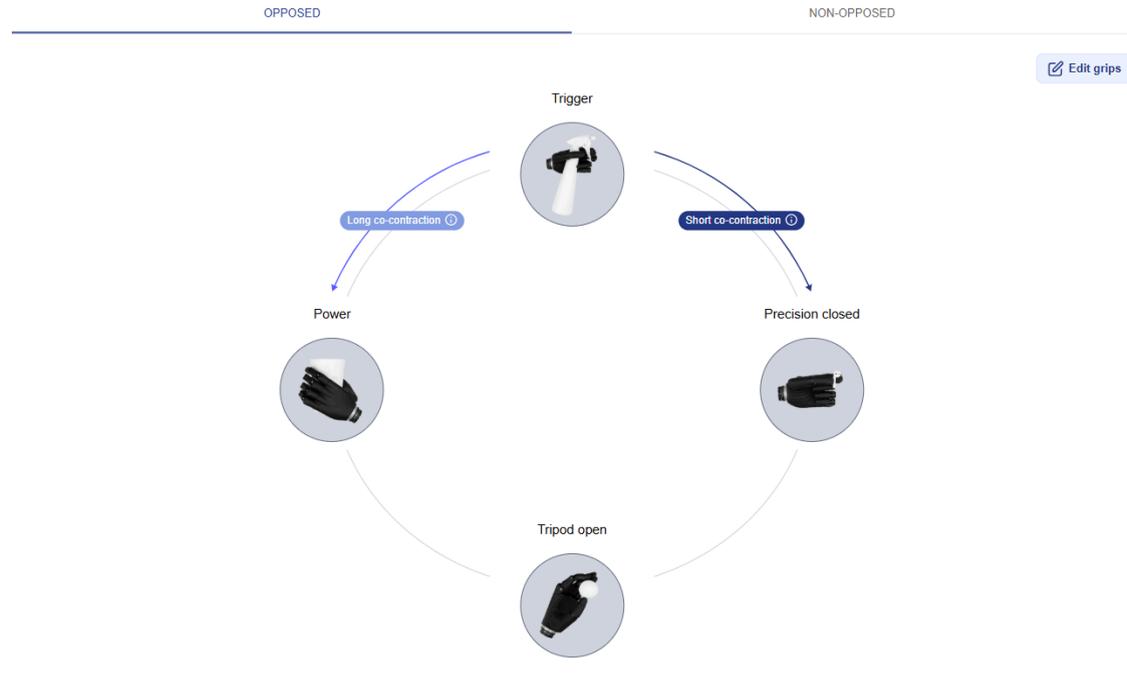

6.2 EMG Settings

EMG ⓘ

ONE SPEED PROPORTIONAL

CS

Open Close

Activation

Open Close

Time: last 25 seconds

Open signal
Gain: 100%

Close signal
Gain: 100%

Smoothness: 0

Smoothness: 0

- In the EMG Setting tab you can see the graph depicting the signals and their strength acquired from the patient's muscles.
- To accommodate varying levels of signal strength and electrode sensitivity, there are special slider adjustments to change the threshold levels for the grip Change Signal and the activation levels to open and close the hand.
- On the left side of the screen there are 2 sliders with a scale. They can be easily adjusted to establish a suitable grip Change Signal threshold for each patient individually.
- On the right side of the screen there are 2 additional sliders. They can be used to adjust a suitable activation level for the open and close signal.
- You can adjust the timescale on the graph by a slider at the bottom of the Settings Area.
- You can hide or show the thresholds on the graph by toggling the checkbox beneath their sliders.
- You can adjust the smoothness of EMG signal
- You can set the gain on the sliders at the bottom of the screen. It is recommended that the gain is primarily set on the electrode first (when applicable), and the slider is used as an adjuster when the electrode adjustability is not available.
- There are a couple of options that affect the appearance of the graphs.

- One Speed- in this option, both muscle signals (Flexion and Extension) are shown on the same graph



- Proportional - this option enables you to change the thresholds for proportional control of the hand. Both of the signals are visible on the same screen. The thresholds are available on the right-hand side of the Settings Area. There is also a special "Full power" threshold which is used for Soft-grip functionality. If you have One speed setting selected, you won't be able to change the threshold for "speed 2" and "speed 3". Also the sliders corresponding to them will be grayed out.



- The threshold bar reflects how high each signal must reach to register as a valid signal. It verifies if the signal the patient made is strong enough to be read and for the hand to start moving.
- If the patient has problems controlling the hand, the threshold bar can be adjusted.

Adjustment	Effect	Consequence
Raising	Patient needs a higher signal in order for the hand to start moving	The user is less likely to have un intended hand movements, but the hand may seem slower as a higher signal needs to be given
Lowering	Patient needs weaker signal for the hand to start moving	It's easier to activate the prosthesis, but there is more potential for inadvertent operation / accidental opening

6.3 Grips configuration tab

- In the Grips configuration tab you can change the initial and end limit positions for each and every grip.
- The initial position of each finger is the position that is assumed after changing to the grip.
- Position limit is the maximum end position the finger can move to while closing. Both of those parameters can be adjusted for each finger individually in every grip; 1000 is fully closed, 0 fully open. This can be used for fine tuning of the grips.
- To begin, you have to select the right grip in the dropdown at the top right corner.
- You can activate the movement of the hand while configuring the grips to see what the finger positions actually look like by checking the box at the bottom right corner.
- As well as the 14 default grips in the Zeus Hand, the Clinician can configure 3 additional Custom Grips for the Patient.

Be aware of the surroundings of the hand while doing this. Try to avoid moving fingers in a way that they might hit other digits, as this may lead to damaging the fingers.

6.4 Choose grips tab

In the upper right corner of the Settings Area you will find the Pairing Mode / Sequential Mode switch. Changing this switch will select the corresponding control mode setting in the prosthesis.

- Choosing the control mode changes the displayed graphics in the Settings Area. There you can select the order in which the grips will be accessed in each of the control modes.


The Zeus has 14 selectable grip patterns. The clinician can choose the grips that are the most useful in the patient's daily life.

Additionally the Clinician can set 3 custom grips for the Patient.

6.4.1 Custom Grips

As mentioned above the Clinician can set an additional 3 custom grips for the patient.

The custom grip function is accessed via the button "Add Custom Grip" button. See image below.

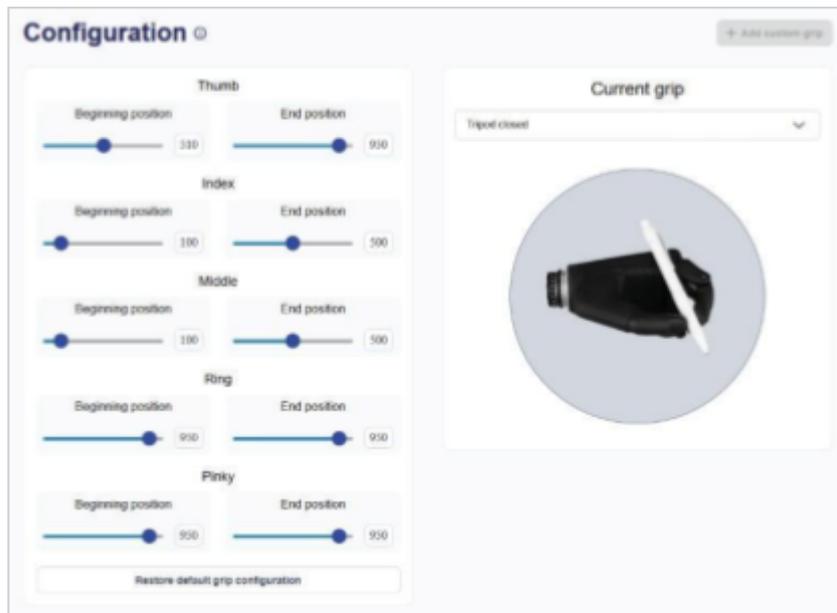

This then opens a window for the Clinician to design a specific grip for the Patient. It can then be named, saved and available for the Patient.

See image below.

The screenshot shows a 'Configuration' window with a title bar and a '+ Add custom grip' button. The main area is divided into two panels. The left panel, titled 'Configuration', contains five rows of controls for different fingers: Thumb, Index, Middle, Ring, and Pinky. Each row has a radio button to toggle the finger's inclusion, followed by 'Beginning position' and 'End position' sliders with numerical values. The right panel, titled 'Current grip', shows a dropdown menu with 'Custom grip 1' selected, a large circular icon with a hand and the text 'Custom grip', and a 'Details' section with a 'Name for the grip' field (containing 'Custom grip 1'), a 'Grip type' dropdown (set to 'Opposed'), and three buttons: 'Remove', 'Save as template', and 'Save details'.


Finger	Beginning position	End position
Thumb	100	806
Index	555	950
Middle	562	617
Ring	100	950
Pinky	100	950

6.5 Prosthesis settings tab

In the Prosthesis settings tab you are able to configure various settings and parameters for the Zeus hand.

6.5.1 Input Options

This refers to the method by which a patient can control the prosthesis.

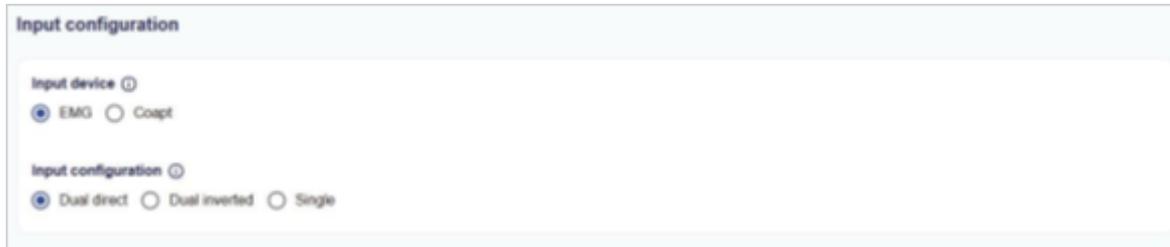

The screenshot shows a web interface for 'Input configuration'. It has two sections, each with a title and a dropdown arrow. The first section is 'Input device' with two radio buttons: 'EMG' (selected) and 'Coapt'. The second section is 'Input configuration' with three radio buttons: 'Dual direct' (selected), 'Dual inverted', and 'Single'.

6.5.1.2 EMG - control the prosthesis using single or dual channel EMG electrodes, or any other device with analog output from 0 to 5V.

6.5.1.3 Pattern Recognition- control the prosthesis using a pattern recognition system which detects the intended grip pattern that the user wants to achieve.

6.5.2 Input Sites

6.5.2.2 The choice of this option depends on the patient's muscle condition, the level of the amputation and their stage in the rehabilitation process. It relates to the production and sending of good quality EMG signals.

- Dual Direct

- Dual Inverted

- Single

6.5.2.3 These options mean the patient can use one electrode or two - in direct or inverted mode - to control the prosthesis.

6.5.2.4 Dual direct mode is the default option, with signals from two electrodes being used to control the prosthesis. Dual inverted mode simply swaps the electrode inputs. The electrode that would close the prosthesis' fingers in the direct mode will open them in the inverted mode.

6.5.2.5 Single electrode mode is designed for patients that cannot use dual modes because of difficulty in producing two differentiable, strong signals.

6.5.3 Speed Control Strategy

In this section, there are 2 options for the speed of the hand:

Speed and strength

Speed control strategy ⓘ
Mode in which you operate the prosthesis

One speed Proportional

Soft-grip ⓘ
Used to limit the strength of the fingers

On Off

Gentle Strong

—————●—————

[Calibration Procedure](#)

Fingers speed calibration ⓘ
Used to set correct fingers speed after repair and firmware update

[Calibration Procedure](#)

6.5.3.2 One speed: One speed control means that once the threshold has been passed, the speed of the hand is always at the same level regardless of the EMG signal strength. The threshold can be changed in the settings.



6.5.3.3 Proportional: control means that speed of the hand is proportional to the patient's EMG signal strength. In this mode the patient has to contract his muscles stronger to move the fingers of the prosthesis faster. There are three achievable speeds; each of them is applied to the prosthesis fingers after exceeding a certain EMG strength threshold.

This section allows the user to select the type of signal used to change the grip. This can either be:

6.5.3.4 Co-contraction (default) is the simultaneous contraction of both muscles used to control the prosthesis. If the co-contraction is shorter than 0.5s, then it is treated as the primary grip Change Signal. Longer co-contractions act as secondary grip Change Signals. The timing that defines the short and long co-contraction can be changed in the software.



6.5.3.5 Open-open grip Change Signal is the sequence of two quick contractions of a muscle used to open the prosthesis. If the time between two such contractions is shorter than 0.5s, it will activate the primary grip Change Signal. To achieve a secondary grip Change Signal, the user needs to perform three muscle contractions in a sequence (open-open-open).

6.5.3.6 In hold-open mode, the patient generates the primary grip Change Signal by keeping the open signal high while the fingers are already fully open for 1.5 seconds and they generate the secondary grip Change Signal by doing the same for 2.5 seconds. These timings can be adjusted by changing the Hold-open grip switching mode sliders.

6.5.3.7 Single electrode grip switching mode is used when only one input / signal is possible. In this mode, the patient can choose between two ways of changing the fingers movement direction:

- **Alternating:** the patient closes and opens the hand with the same signal. The first generation of the signal closes the fingers, the second generation of the signal opens the fingers. Double short impulse of the signal is used for a primary grip Change Signal and triple short impulses are used for a secondary grip Change Signal.
- **Slope:** the speed at which the patient increases the signal strength defines the movement direction. Increasing the signal slowly causes the hand to close. Fast increase in signal strength causes the hand to open. To change a grip, the user needs to hold the opening signal, while the fingers are fully open.

6.5.4 Grip switching settings

These settings will appear when correct grip switching mode is selected

Grip control

Grip switching modes ⓘ
Different ways of generating Charge Signal (CS) and Secondary Charge Signal (SCS)

Co-contraction Open-open Hold open

Co-contraction settings ⓘ
Auto length of co-contraction signal

Long co-contraction time

0.50s

Signal rise offset time

0.10s

EMG freeze mode switch ⓘ
Enables or disables EMG freeze mode for the patient using EMG signals.

Enabled Disabled

Following grip ⓘ
Enables or disables following grip

On Off

Ignore EMG spikes ⓘ
Ignore short noise spikes of the specified length.

On Off

Time ignored:

0.30s

Co-contraction - Co-contraction timings. Long co-contraction time allows you to specify the time after which holding a co-contraction signal is treated as a secondary grip Change Signal. Signals shorter than this value are treated as the primary grip Change Signal. The signal rise offset time slider allows you to specify the maximum time between two signals crossing the CS threshold to be treated as a grip Change Signal.

Open-open and single electrode alternating - Pulse timings. Minimum and maximum pulse time slider allows you to specify which length of the signal impulses will be treated as valid. The minimum time between pulses slider allows you to specify precisely this so that noisy signals won't be treated as multiple pulses. The maximum time defines at what time the hand stops waiting for a second signal - important for daily use and remembering there may even be a third open signal.

Hold-open - hold-open timings. In these settings there are two sliders used for specifying the time for primary Change Signal and secondary Change Signal.

6.5.5 Soft-Grip

The strength of the fingers can be limited by the soft-grip functionality. It adjusts the maximum grip force applied by the hand on an object. It also enables you to specify an additional threshold for the EMG closing signal, which once exceeded, restores the full strength. By default then, the patient can have a very light touch, but likewise can squeeze and even squash an object if desired. When enabling this function, you need to calibrate the fingers by pressing the Calibration procedure button.

Warning!

Keep your hand in a safe position while calibrating as its fingers will be moving.

6.5.6 Finger speed calibration

For hands that have firmware version 2.1 or greater Finger speed calibration will calibrate all fingers to match the slowest finger speed. This should be done after a finger is replaced, or there might be visible speed difference between the fingers.

Once the Calibration procedure button is pressed the fingers will move to calibrate. Once complete, a table with information status will be displayed.

If the hand has firmware version prior to 2.1 the finger calibration will not be displayed.

Note: In asynchronous session: Finger speed calibration can't be performed during asynchronous session, because the device is not connected.

6.5.7 Ignore EMG spikes

If the patient is facing difficulty with EMG spikes - for example while exercising - you can activate the "ignore EMG spikes" function. By doing this, the prosthesis will ignore short spikes of EMG of the length specified by the adjustable slider.

Keep in mind that this function will create a delay in the prosthesis response time, as the initial part of the signal is ignored. With this selected, the timing parameters of open-open may need to be adjusted to allow for intentional grip switching.

6.5.8 EMG freeze mode

When the option is turned on the fingers will not move at all until the Change Signal (CS) is given

6.5.9 Audio & vibration signal guide

This section provides detailed explanations of each audio and vibration signal. It includes information on the circumstances under which each signal is activated, its duration and frequency.


See the table below for the detail of each parameter.



- 6.5.9.2** **Feedback settings:** Allows the clinician to set the type of feedback the patient will get from the hand. The feedback is given on various events like passing hold-open Change Signal time, warning about low battery level etc.
- **Audio** - the hand will notify the user using audible beeps. Volume of the beeps can be adjusted using the slider
 - **Vibration** - the hand will vibrate to notify the user. The strength of the vibrations can be adjusted using the slider. This option may not be available in some versions of the hand.

Notification pattern	Meaning
Two while holding signal	About to enable/disable freeze mode
One long notification	Freeze mode enabled
One (while holding opening signal)	Hold open
One (while no signals are present)	Movement direction change (single electrode)
Two repeated every 30s	Low battery alarm (low priority)
Three repeated every 5s	Low battery alarm (medium priority)


7 DEVICE USAGE MONITORING - DUM

Device usage monitoring provides information regarding day-to-day use of the prosthesis by the patient. It consists of graphs that present information such as the number of performed grips and grips switches, together with hourly breakdown.

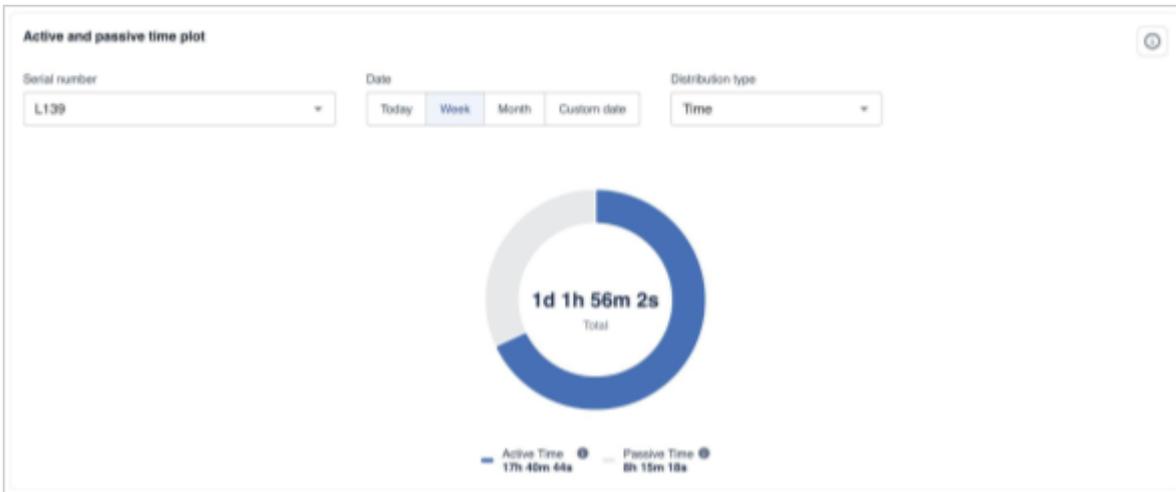

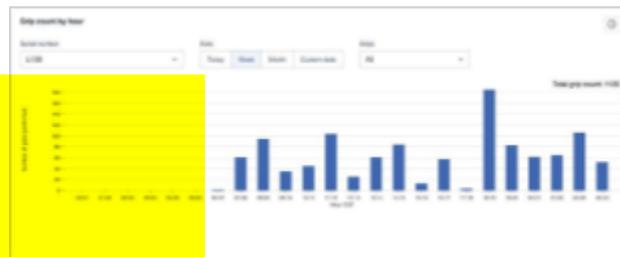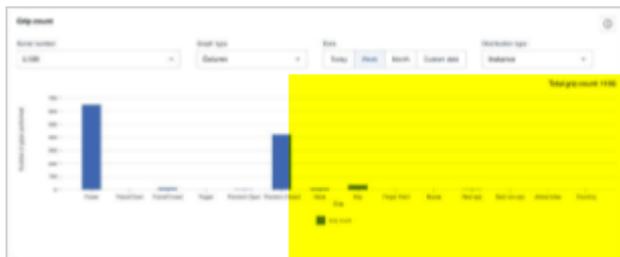

8 MODES

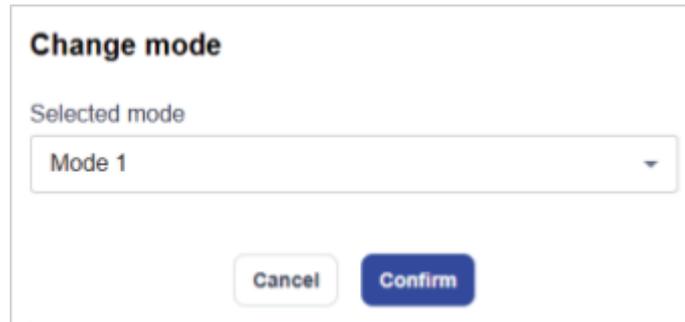

The image shows a dialog box titled "Change mode". Inside the dialog, there is a label "Selected mode" above a dropdown menu. The dropdown menu currently displays "Mode 1" with a small downward arrow on the right side. Below the dropdown menu, there are two buttons: a light blue "Cancel" button and a dark blue "Confirm" button.

Modes represent different configurations saved in the device. Use this feature to create different setting modes for patients. This can be used for sports, vocation, recreational activities, etc. This can be done using modes. After the clinician creates mode profiles, they are sent to the patient's hand for use. The patient will be able to switch between modes on their mobile app. They can be switched using the dropdown visible in the upper-center part of the screen.

Modes allow you to set different hand configurations, which the patient can switch with one click from the mobile app. All mode settings are separate, e.g. Mode 1 can have different grip settings than Mode 2. There are a maximum of 3 modes per device. In the panel on the right in Configurator you can choose which mode you are currently editing.

Each mode holds the following parts of configuration:

- Grips pairs/grips sequence
- EMG settings
- Speed control strategy
- Grip switching mode
- Co-contraction/pulse/hold-open timings
- Ignore EMG spikes settings
- Soft-Grip settings

The remaining configuration elements are not stored in the mode and as such are common for all modes

- Grips fingers position

Select a mode that you would like to use and make a change to the hand configuration that will be stored in the new mode. Once the change is made, hit the send to prosthesis button. This can be done locally, asynchronously or during remote sessions.

9 ALLIED HEALTH

Allied Health can use other functionalities on the same rules as Clinicians after granted access. the description of the functionalities you can find under section: Remote session, Local Session, Asynchronous session, Config template, Modes, Goals, History log.


9.1 Allied Health permissions

Allied Health in the application has specific access to selected patients and functionality depending on the permission granted by the Clinician.

Permissions to ADP and Zeus Configurator


- Grips
 - Change grips
 - Transition mode
 - Grips configuration
- EMG settings
- Main settings
- Goals
- Soft grip
- Speed control strategy
- Other settings

9.2 Allied Health – My patients

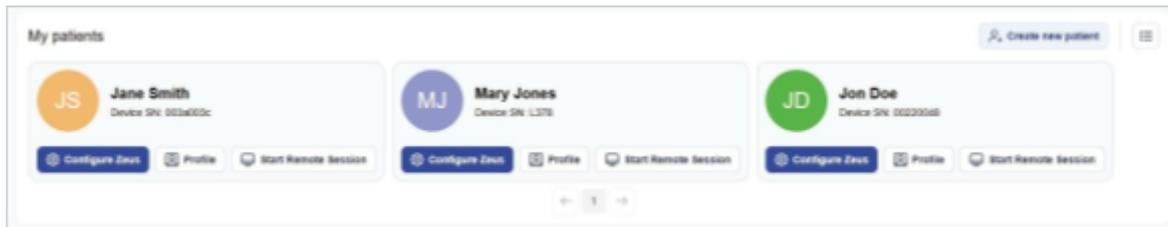

This view shows a list of patients for whom access has been granted by the Clinician.


The full view of the patient's information is available by clicking the button "Profile" on the Patient Card.

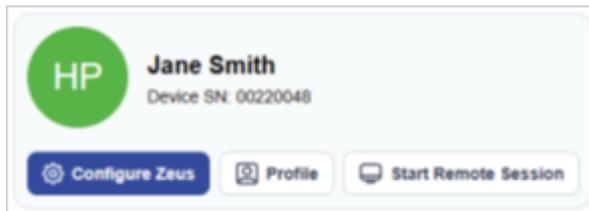

10 TECHNICAL SUPPORT

10.1 Troubleshooting

Device -ADP firmware version mismatch



Mismatch happens when the device's firmware version is different from the one ADP expects. It might mean that the device was updated outside of the ADP.

10.1.1 Configuration not found:

Shown when the device has not been connected yet, either to the web or mobile application. Without configuration initiated, session and async configuration modes stay disabled.



10.1.2 Upgrade needed:

The device's firmware is not updated to the latest version so that features may not work correctly. In specific situations, the clinician may be locked out of all configurator features until firmware is updated.



In the case of any issues with the software:

Check if the hand is turned ON
Check if the battery is charged

If a problem initiating Bluetooth connection occurs, the following error will be displayed. In such a case try refreshing the page, check the device's battery level, turn it off and on again, and try connecting once more.



If the firmware will become unresponsive, during initial connection a popup will appear asking you to update the device. Configuration can't be changed locally until firmware update is installed successfully in such a case. In the event of a firmware update failing repeatedly please contact Aether support.

In the email message the user should specify a question or a problem that has occurred, preferably describing what led to it, what is happening and what a desired outcome would be.

- The bluetooth ID is not detected? Reopen your browser and connect with the hand.

Screenshots as attachments can be included to increase the speed in resolving a problem.

10.1.3 Firmware Update

The Clinician may update the firmware on the Patients Zeus Hand via the ADP. To access this feature, navigate to Patients profile and:

10.1.3.2 Start a Remote Session with Patient or

10.1.3.3 Start a Local Session with Patient

During Session (Remote or Local) in the Configurator please go to Firmware update tab and follow information on screen below.

10.1.4 WIFI

IOS can turn off wifi by itself in some cases if not used for a long time or to save battery. Due to that there is a possibility that notification will be delayed or not received at all. Please check if WiFi connection is present and Turn OFF and then Turn ON once again.

10.2 Compatibility

The Aether Digital Platform is compatible with Zeus V1 hands A-01-L/R; A-01-L/R-T; A-01-L/R-TS-S/A02L-SF0B;A02R-SF0B.

10.3 Reporting

Any serious incident that has occurred in relation to the device should be reported to Aether Biomedical Sp z o.o. via support@aetherbiomedical.com and the competent regulatory authority of the country in which the user is a resident.

10.4 Security

Application should be operated from a secure device. It should have the firewall enabled and have anti-malware software installed.

It is recommended to check the certificate of the web page before logging in.

It is recommended to close the application when you are not using it or you are away from the computer.

11 OTHER INFORMATION

- Aether Biomedical declares that they meet appropriate European standards for design, manufacture and supply of prosthetic products and user software under CE mark. Continued compliance with the standard is monitored by a program of internal and external audits.
- All individual products are marked indicating that they comply with the requirements of the Medical Device Regulation 2017/745.

11.1 Symbols



This CE mark indicates the product conforms with the essential requirements and provisions of Medical Device Regulation 2017/745.

Refer to operating instructions



This mark indicates the user should read the operating instructions before use.



This indicates www.aetherbiomedical.com.

Definitions

User: Clinician, Clinic Admin, Allied Health ADP:
Aether Digital Platform

AETHER

B I O M E D I C A L

www.aetherbiomedical.com



Aether Biomedical Sp. z o.o.

ul. Mostowa 11, 61-854

Poznań

POLAND

Phone:

POLAND+48780011548

INDIA +91 9636842365

USA +1 4708238221

e-mail: info@aetherbiomedical.com

© Copyright Aether Biomedical 2025. All rights reserved.